

NANO ZS



Size Distribution Report by Volume

Sample Details

Sample Name: Meditech Europe CS

SOP Name: NarrowHighRes.sop

General Notes:


File Name:	CSL-2010-size.dts	Dispersant Name:	Water
Record Number:	744	Dispersant RI:	1.330
Material RI:	1.25	Viscosity (cP):	0.8872
Material Absorbtion:	0.01	Measurement Date and Time:	Thursday, August 12, 2010 ...

System

Temperature (°C):	25.0	Duration Used (s):	60
Count Rate (kcps):	300.3	Measurement Position (mm):	4.65
Cell Description:	Disposable sizing cuvette	Attenuator:	9

Results

	Diam. (nm)	% Volume	Width (nm)
Polydispersity Index: 0.609	Peak 1: 13.82	92.3	1.9
	Peak 2: 81.28	2.2	17.7
	Peak 3: 485.13	0.5	103.8

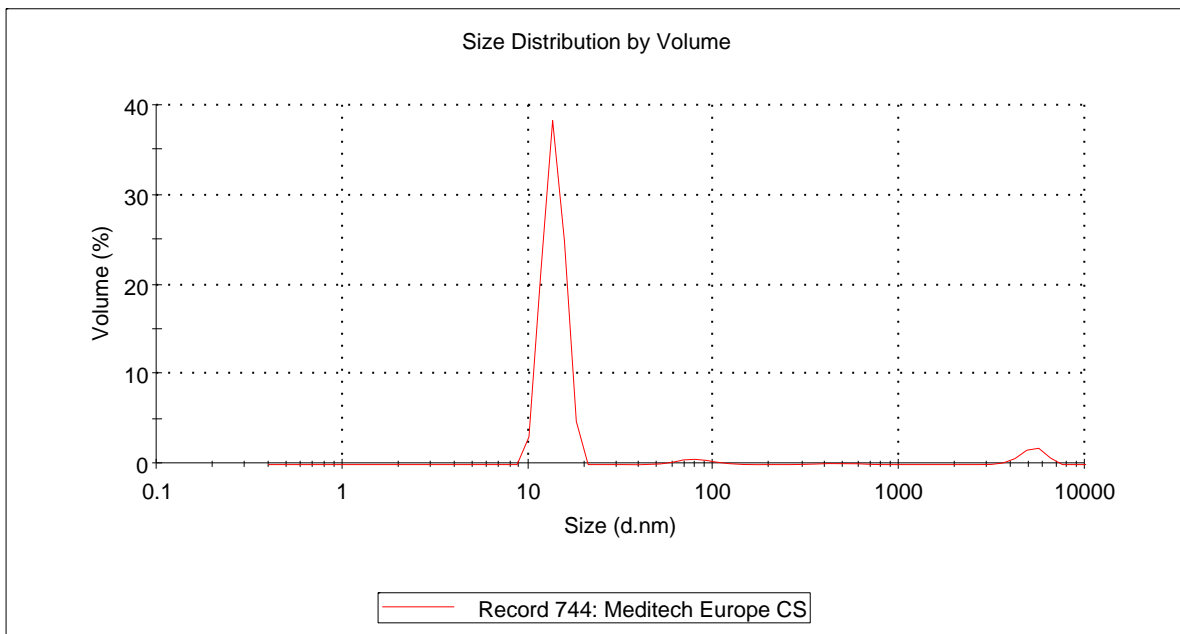

Colloidal Science Laboratory, Inc.

Westampton, NJ 609-267-2065