

NANO ZS



Size Distribution Report by Volume

Sample Details

Sample Name: SanteNaturels20-15006A-Post14k3mSpin
SOP Name: CSL-ms.sop
General Notes: Average result created from record number(s): 1085 1088 1089 1093


File Name: CSL 2015.dts
Record Number: 139
Material RI: 1.25
Material Absorbtion: 0.010
Dispersant Name: Water
Dispersant RI: 1.330
Viscosity (cP): 0.8872
Measurement Date and Time: Monday, June 22, 2015 12:4...

System

Temperature (°C): 25.0
Count Rate (kcps): 351.7
Cell Description: Disposable sizing cuvette
Duration Used (s): 60
Measurement Position (mm): 4.65
Attenuator: 9

Results

	Diam. (nm)	% Volume	Width (nm)
Polydispersity Index: 0.809	Peak 1: 0.67	99.0	0.1
	Peak 2: 2.63	1.0	0.6
	Peak 3: 0.00	0.0	0.0

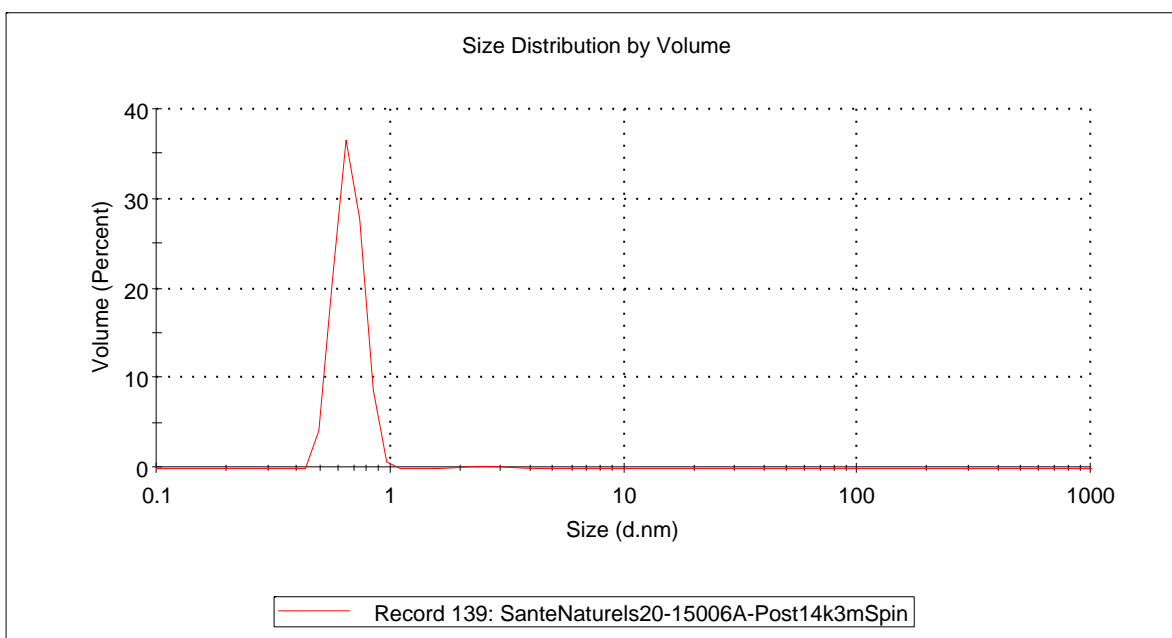

Colloidal Science Laboratory, Inc.

Westampton, NJ 609-267-2065