

# NANO ZS



## Size Distribution Report by Volume

### Sample Details

Sample Name: TecnoSalute

SOP Name: NarrowHighRes.sop

General Notes:


File Name: CSL-2011-size.dts      Dispersant Name: Water  
Record Number: 6      Dispersant RI: 1.330  
Material RI: 1.25      Viscosity (cP): 0.8872  
Material Absorbtion: 0.01      Measurement Date and Time: Thursday, March 03, 2011 4...

### System

Temperature (°C): 25.0      Duration Used (s): 70  
Count Rate (kcps): 459.1      Measurement Position (mm): 4.65  
Cell Description: Disposable sizing cuvette      Attenuator: 11

### Results

	Diam. (nm)	% Volume	Width (nm)
<b>Polydispersity Index:</b> 0.340	<b>Peak 1:</b> 56.83	45.5	8.3
	<b>Peak 2:</b> 206.15	54.5	44.8
	<b>Peak 3:</b> 0.00	0.0	0.0

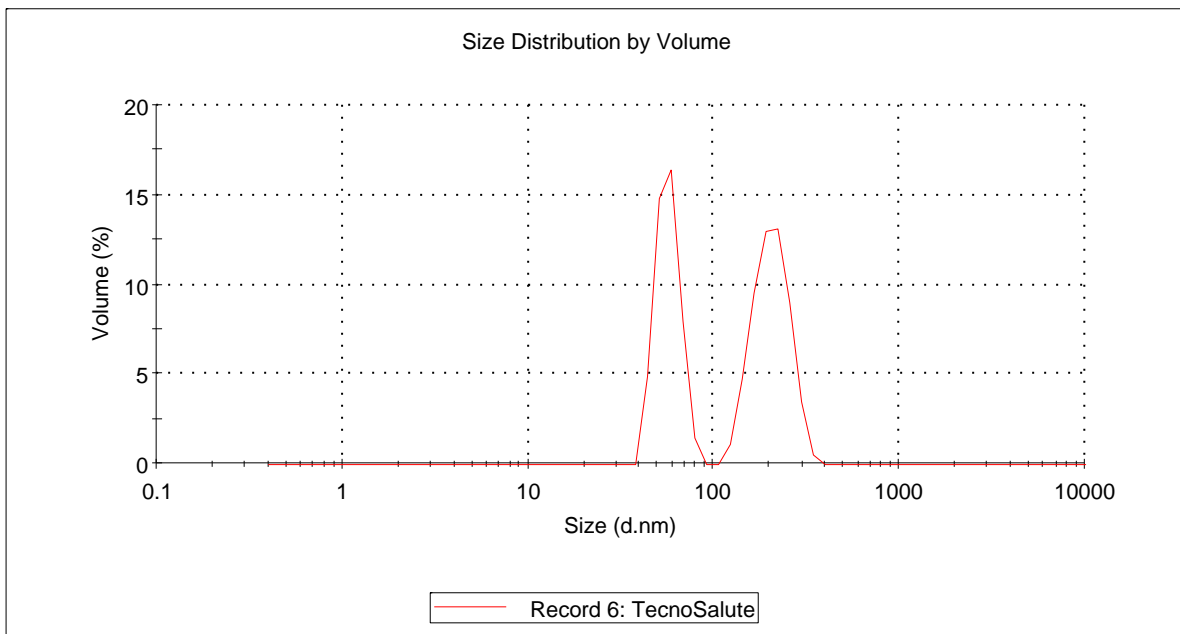

Colloidal Science Laboratory, Inc.

Westampton, NJ 609-267-2065