

NANO ZS



Size Distribution Report by Volume

Sample Details

Sample Name: Harmonik -CS

SOP Name: NarrowHighRes.sop

General Notes:


File Name: CSL-2010-size.dts Dispersant Name: Water
Record Number: 722 Dispersant RI: 1.330
Material RI: 1.25 Viscosity (cP): 0.8872
Material Absorbtion: 0.01 Measurement Date and Time: Tuesday, August 10, 2010 4...

System

Temperature (°C): 25.0 Duration Used (s): 60
Count Rate (kcps): 279.1 Measurement Position (mm): 4.65
Cell Description: Disposable sizing cuvette Attenuator: 9

Results

	Diam. (nm)	% Volume	Width (nm)
Polydispersity Index: 0.138	Peak 1: 120.83	100.0	30.6
	Peak 2: 0.00	0.0	0.0
	Peak 3: 0.00	0.0	0.0

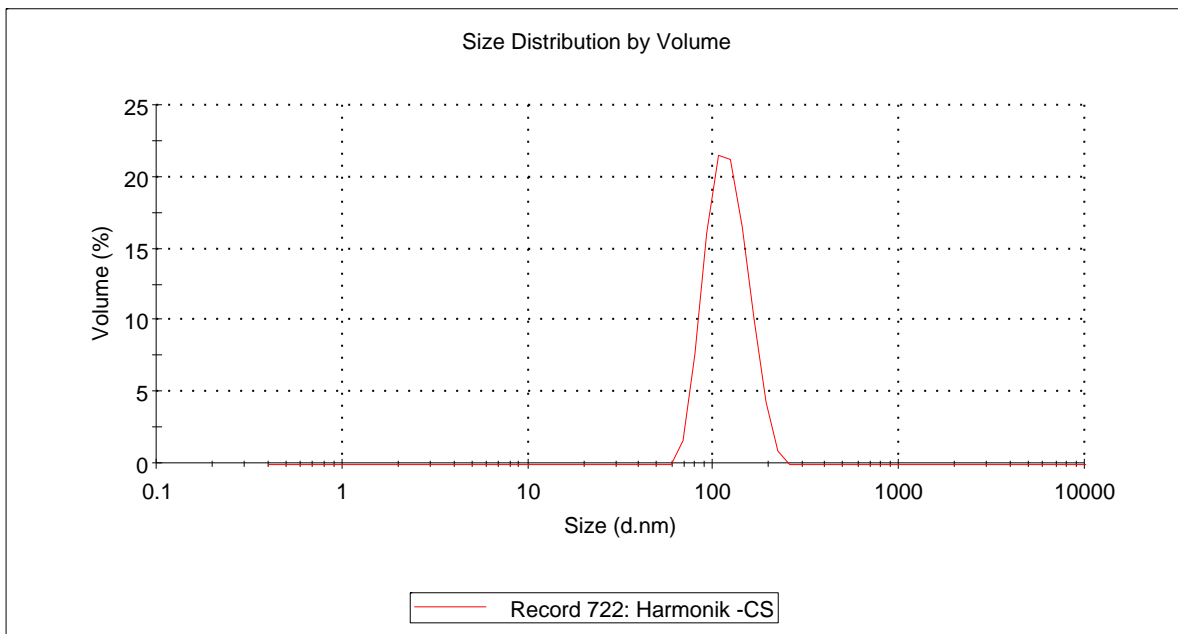

Colloidal Science Laboratory, Inc.

Westampton, NJ 609-267-2065