

NANO ZS



Size Distribution Report by Volume

Sample Details

Sample Name: Home brewed w/ SG-7

SOP Name: CSL-01.sop

General Notes:


File Name: CSL-size.dts	Dispersant Name: Water
Record Number: 459	Dispersant RI: 1.33
Material RI: 1.25	Viscosity (cP): 0.8872
Material Absorbtion: 0.01	Measurement Date and Time: Thursday, April 14, 2005 2:2...

System

Temperature (°C): 25.0	Duration Used (s): 60
Count Rate (kcps): 308	Measurement Position (mm): 4.65
Cell Description: Disposable sizing cuvette	Attenuator: 10

Results

	Diam. (nm)	% Volume	Width (nm)
Polydispersity Index: 0.252	Peak 1: 27.56	71.4	5.2
	Peak 2: 111.25	28.6	26.1
	Peak 3: 0.00	0.0	0.0

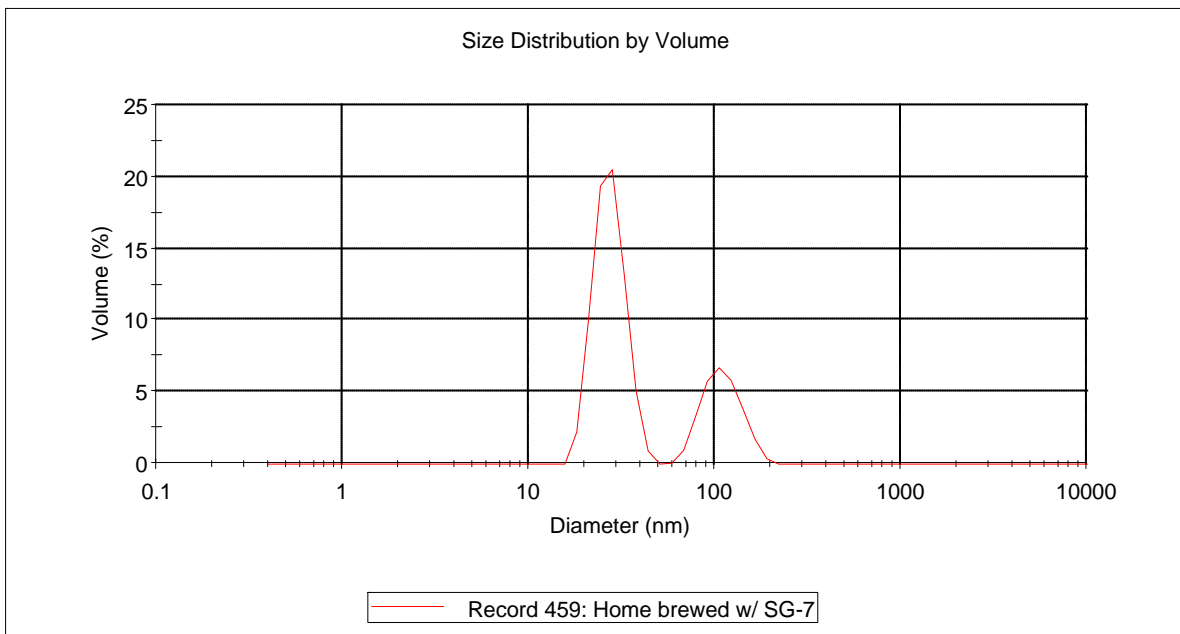

Colloidal Science Laboratory, Inc.

Westampton, NJ 609-267-2065