

HPPS



Size Distribution Report by Volume

Sample Details

Name: Silver Wain Water

SOP: csl-01.sop

Notes:

Filename: CSLResults.dts

Record: 20

Material RI: 1.25

Absorption index: 0.01

Dispersant: Water

Dispersant RI: 1.33

Sample visc. (cP): 0.8872

Date and Time: Wednesday, April 14, 2004 7:...

System

Temperature (°C): 25.0

Cell type: Disposable sizing cuvette

Count rate (Kcps): 46

Meas. position (mm): 2.00

Run duration (s): 10

Attenuation index: 11

Results

Polydispersity index: 0.916

Peak 1 Mean: 6.263

% (Volume): 95

Width: 0.7474

Peak 2 Mean: 29.48


% (Volume): 2

Width: 5.845

Peak 3 Mean: 2562

% (Volume): 1

Width: 271.4

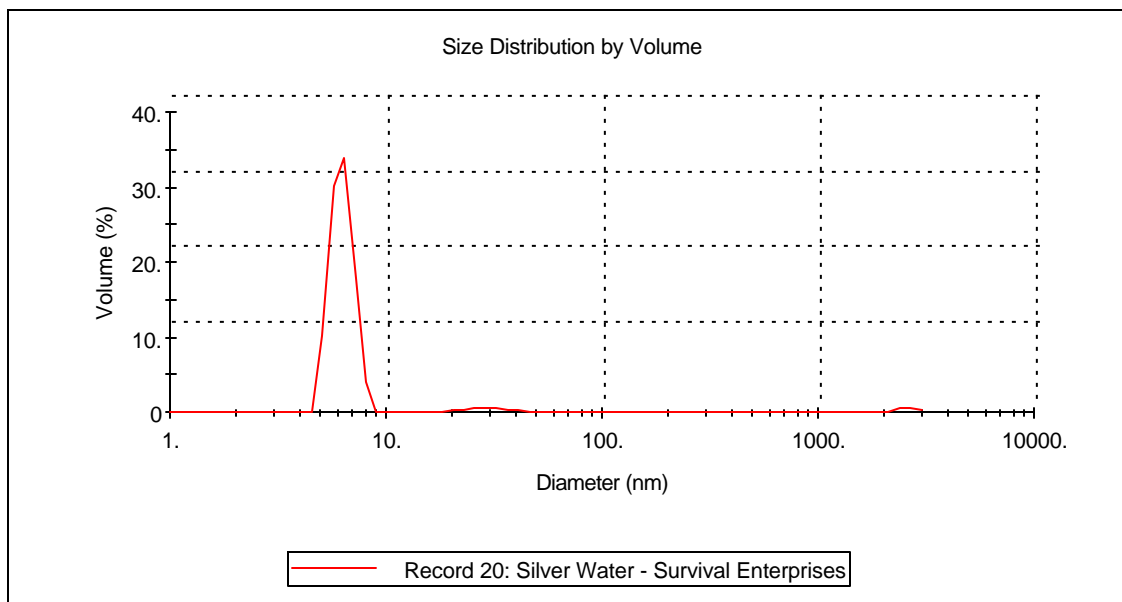

Colloidal Science Laboratory, Inc.

Westampton, NJ 609.267.2065